Absorgyn Gynaecological towels and rectangular absorbent insert

The outer layer made of soft nonwoven.
The inner layer comprises nonwoven and cellulose absorbent core, which ensures high absorption properties.
Film placed between the nonwoven and the cellulose serves as an isolating part – effectively protects against soaking through (in version with film).

Application:

- Products are used to absorb secretions and increase hygiene and comfort in woman in postpartum period or after gynaecological procedures and surgeries.
- Size 35 cm x 11 cm – rectangular absorbent insert for postpartum women and for people with light incontinence.
- Sterile insets are designed to absorb liquids and discharge after delivery or urological and gynaecological procedures.

Types:

- sterile and non sterile
- with or without film
- rectangular and anatomical


Size and packing:

- available sizes: 22 cm x 9 cm, 27 cm x 7.5 cm, 28 cm x 9 cm, 34 cm x 9 cm, 35 cm x 11 cm,
- sterile: packed by 10 pcs or by 5 pcs
- non sterile: packed by 10 pcs, 15 pcs (size 35 cm x 11 cm) and by 20 pcs (size 22 cm x 9 cm)



Rectangular version / Rechteckige Version / Прямоугольная версия / Prostokątna wersja

Method of use / Anwendungsweise / Способ применения / Sposób użycia:

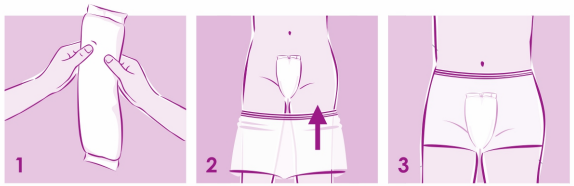


Towels should be changed regularly. / Die Vorlagen sollten regelmäßig gewechselt werden. / Прокладки следует регулярно менять. / Podkłady należy zmieniać regularnie.

The manufacturer recommends stabilisation with Seni Fix elastic supporting briefs. / Der Hersteller empfiehlt die Fixierung mit den elastischen Höschen von Seni Fix./ Производитель рекомендует использовать сетчатые трусики-фиксаторы Seni Fix для закрепления изделия. / Producent zaleca stabilizację za pomocą majtek siatkowych Seni Fix.

Anatomical version / Anatomische Version / Анатомическая версия / Anatomiczna wersja

Method of use / Anwendungsweise / Способ применения / Sposób użycia:

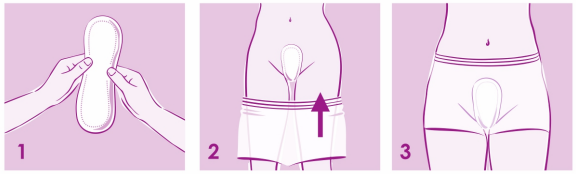

Towels should be changed regularly. / Die Vorlagen sollten regelmäßig gewechselt werden. / Прокладки следует регулярно менять. / Podkłady należy zmieniać regularnie.

The manufacturer recommends stabilisation with Seni Fix elastic supporting briefs. / Der Hersteller empfiehlt die Fixierung mit den elastischen Höschen von Seni Fix./ Производитель рекомендует использовать сетчатые трусики-фиксаторы Seni Fix для закрепления изделия. / Producent zaleca stabilizację za pomocą majtek siatkowych Seni Fix.






MD

Sterile devices are certified by the Notified Body TÜV Nord Polska Sp. z o.o. and bear the CE mark with number 2274

>>

©Copyright 2026 en.matopat-global.com | Last updated: 04.11.2026

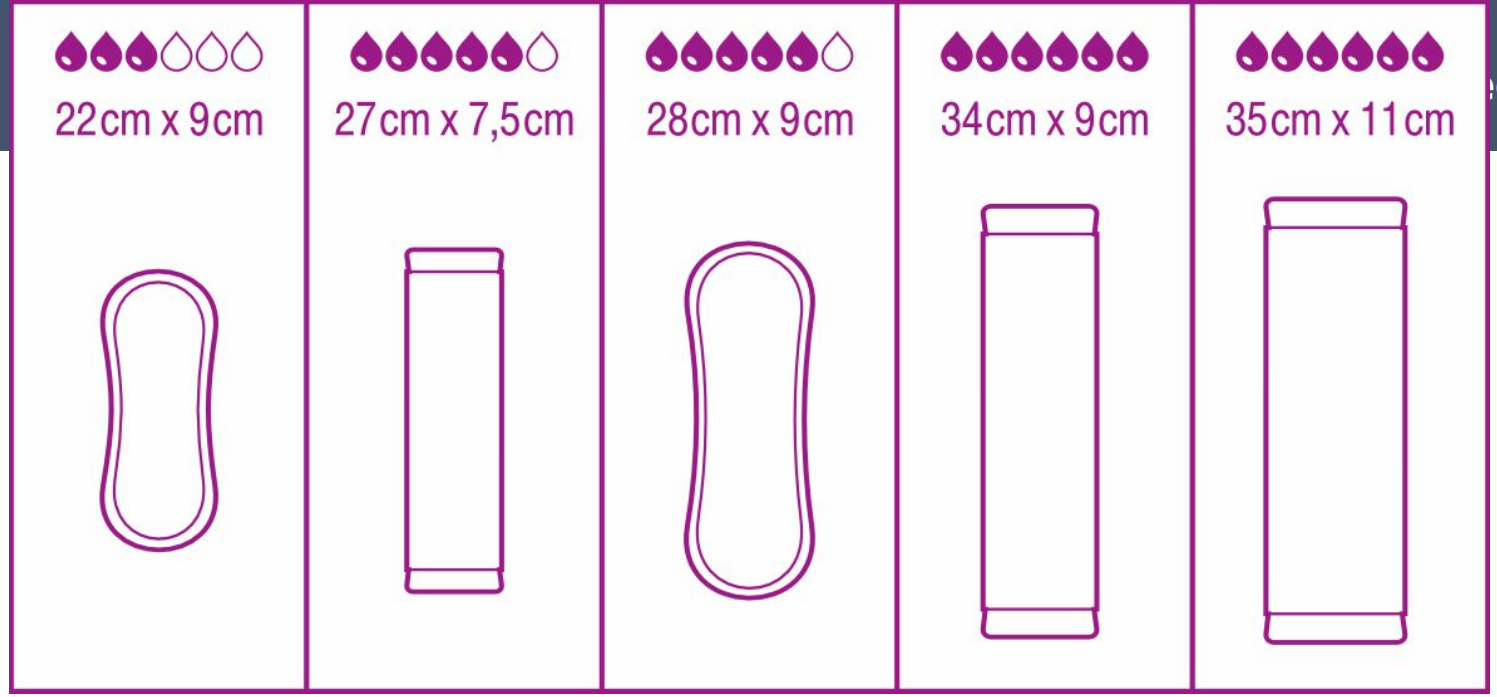

©Copyright 2026 en.matopat-global.com | Last updated: 04.11.2026